

## Accessories



### CHIROBLOC Ballast - ref. CBL

It is an independent spare part made out of stainless steel, it may be attached to CHIROBLOC to weigh it.

Weight: 0.725 kg  
5 years warranty.




### RING - ref. RING

RING will be used as an attachment to any CHIROBLOC.

Sold separately by box of 10 units.  
Warranty: 1 year

RING will replace rubber bands made from surgical gloves.

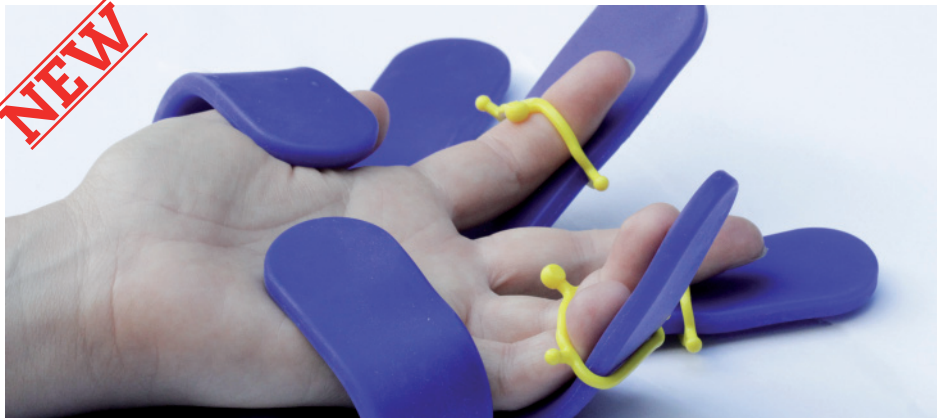

Design: e-monceaux.fr / 252 éd.05 - © AREX® - 2020


## CHIROBLOC3 - ref. CHIRO3

Made out of a composite bio-compatible material.  
Radio-lucency without lead weight.  
Will not stain surgical gloves.

- One wrist band:  
two possible adjustments

Wrist strap /  
child positioning

Wrist strap /  
adult positioning

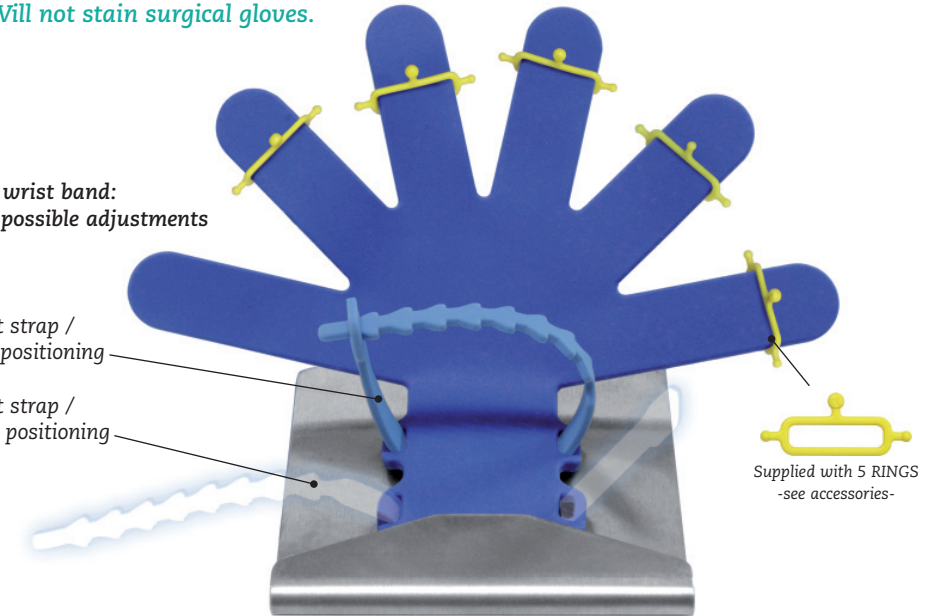


CHIROBLOC Ballast - see accessories

### CHIROBLOC3

Supplied with 5 RINGS

Weight: 0.27 kg

Warranty: 1 year

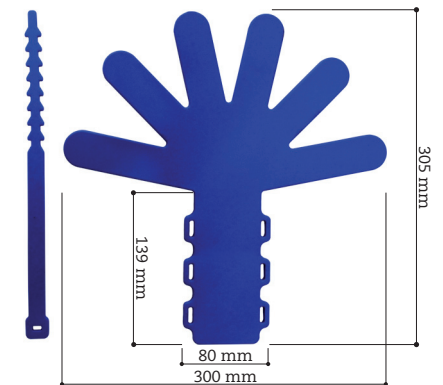


DISTRIBUTED BY



Manufacturer:  
AREX®  
3 allée du Clos Tonnerre  
91120 Palaiseau - FRANCE

[www.arex.fr](http://www.arex.fr)

CHIROBLOC3 & Mini-open CTR

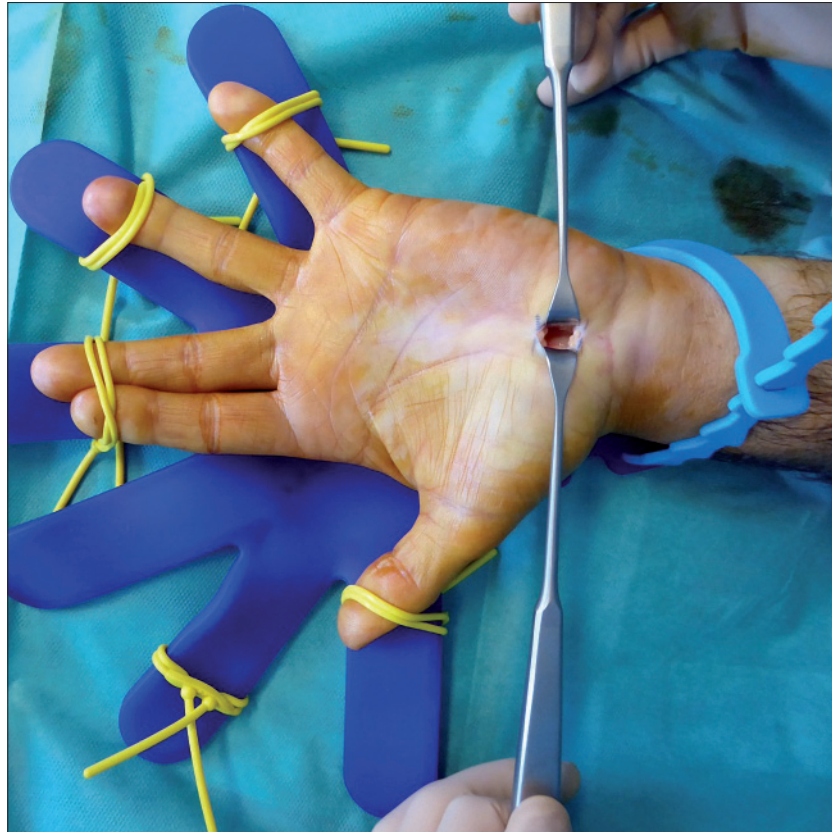

Philippe Liverneaux MD - Strasbourg University Hospital - France

CHIROBLOC3 & Endoscopic CTR



Didier Fontes MD - Paris, Clinique du Sport - France