





# Volar Fixed Angle Plate


Surgical Technique | *TriMed Wrist Fixation System*

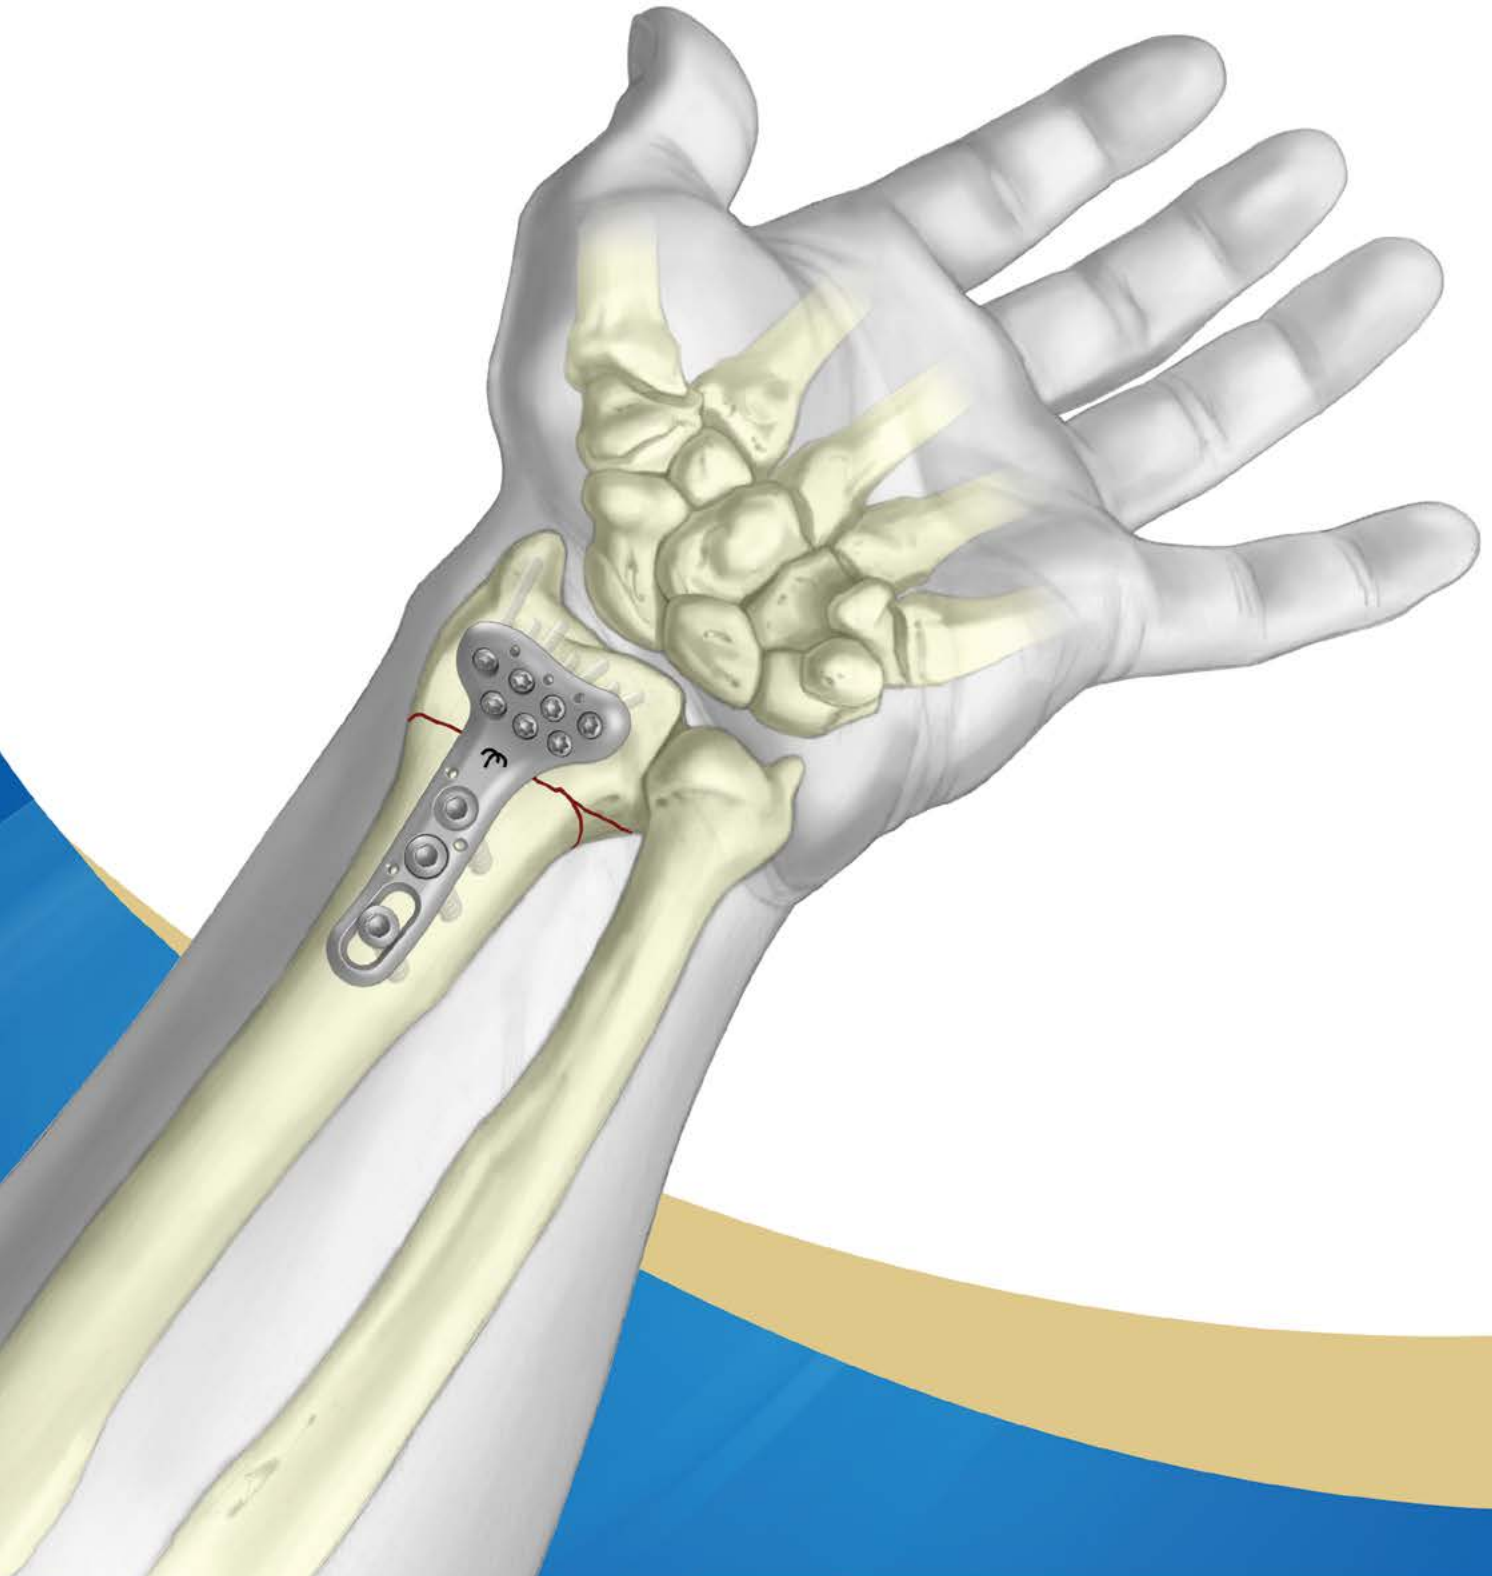

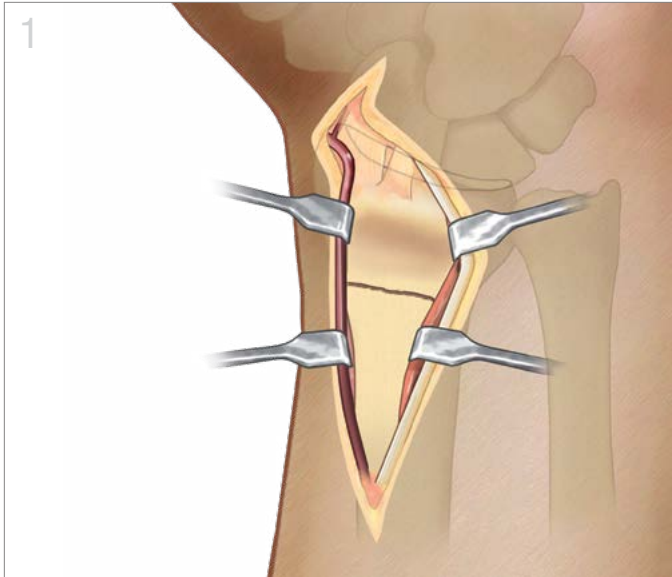


## Exposure (Standard or extended FCR approach)

- Through the distal limb of a modified Henry volar approach, continue the dissection between the FCR and the radial artery.
- Expose the radial shaft by reflecting the pronator quadratus from its radial and distal insertions.
- If needed, release the distal portion of the brachioradialis.

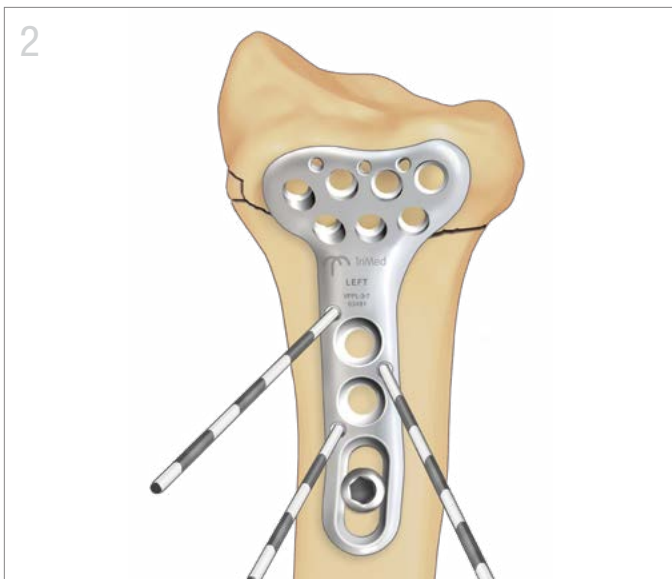


## Fracture Reduction and Provisional Fixation

- Reduce the fracture manually. Transtyloid K-wires may be used for provisional fixation.
- Align plate along the radial border of the radial shaft.
- Secure with 1.1 mm (0.045") K-wires proximally and check position, or fix with a 3.2mm cortical screw in the slotted hole.

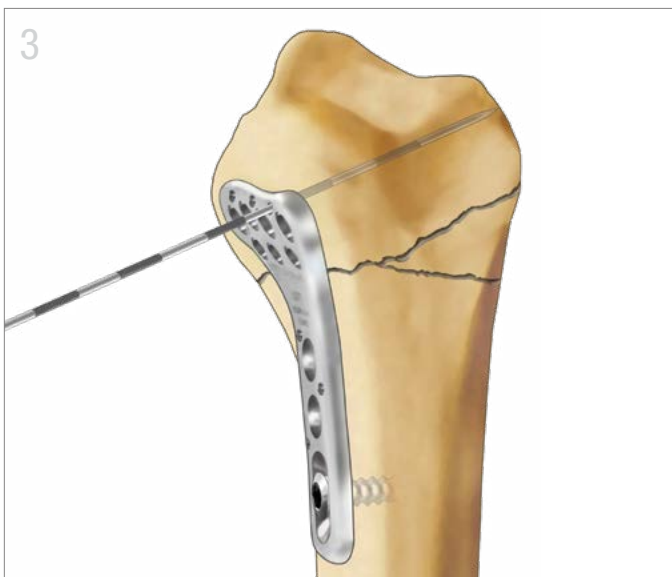

## Confirm Plate and Peg Positions

- Insert a 1.1 mm (0.045") K-wire into a distal pinhole.
- Check the position of the K-wire with the C-arm.
- The K-wire should be directed toward the dorsal rim, and buttress the subchondral bone behind the articular surface.

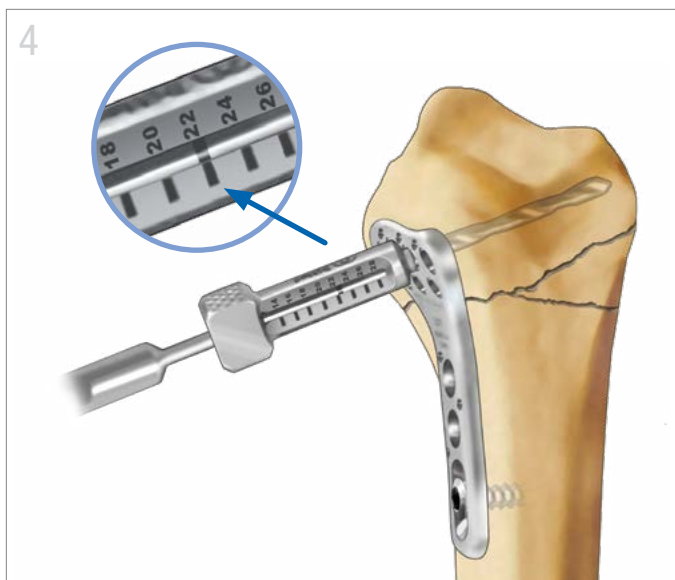

## Peg Preparation

- Thread Peg Guide into a distal peg hole.
- Drill a peg hole using the 1.8mm (blue) drill bit, and measure peg depth with the guide.
- Remove the guide and insert a threaded or smooth locking peg.

**Note:** When using locking drill guides or quick guides ensure installment and placement is concentric to the screw hole. Off-axis guide placement can result in screws not locking into the plate; locking screws can only be used on-axis.



## Final Fixation






- Complete fixation with additional pegs distally and screws proximally.
- Confirm that all screws and pegs are fully seated prior to closing incision.

 Indications, contraindications, warnings and precautions related to TriMed Volar Fixed Angle Plates™ reference IFU, LC-73-2004-003.

## TIPS

1. A Quick Guide can be used in lieu of the standard screw-in Peg Guide for drilling and measuring peg holes.
2. The Plate Benders may be used to contour the plate to the site of application, however, this may alter the trajectory of the fixed pegs.

All implants made from surgical grade stainless steel

Screw Table					
	Unthreaded Peg, 1.8mm	Threaded Peg 2.3mm	Cortical Screw, 2.3mm	Cortical Screw, 3.2mm	Locking Screw, 3.2mm
	UPEG-XX	TPEG-XX	TRX2.3-XX	HEX3.2-XX	LHEX3.2-XX
Length	14-28mm *	14-32mm *	10-32mm *	08-20mm* 11-15mm**	10-20mm *
Drill	● 1.8mm		● 2.3mm		
Guide	GUIDEPEG-1.8		GUIDE-1.8/2.3	GUIDE-2.3/3.2	GUIDEQ-2.3
Driver	Torx 8			2.5mm HEX	

\* 2mm increments \*\* 1mm increments

### Volar Fixed Angle Plate

- STANDARD
- VPPL-3-7
- VPPL-5-7
- VPPR-3-7
- VPPR-5-7



### Peg Guide

GUIDEPEG-1.8



### Quick Guide

GUIDEQ-1.8  
GUIDEQ-2.3



TriMed, Inc. / 27533 Avenue Hopkins / Valencia, CA 91355 USA / 800-633-7221 / www.trimedortho.com

The presently issued U.S. patents are: 6,113,603; 7,037,308; 7,044,951; 7,195,633; 7,540,874; 7,942,877; 8,177,822; 8,821,508; 8,906,070; 9,089,376; 9,283,010; 9,220,546; 9,237,911; 9,402,665; 9,636,157; 9,861,402. See [trimedortho.com](http://trimedortho.com) for all listed patents.

The technique presented is one suggested surgical technique. The decision to use a specific implant and the surgical technique must be based on sound medical judgment by the surgeon that takes into consideration factors such as the circumstances and configuration of the injury.

This document is controlled by TriMed, Inc. When downloaded, printed, and/or copied, this document becomes uncontrolled, and users should always check [trimedortho.com](http://trimedortho.com) for the latest version.

